

Effect of Addition of ZrO₂ on Biaxial Flexural Strength of Calcium Phosphate Ceramics

Mohammed K. Hilal BDS, MSc., Ph.D. ⁽¹⁾

Mohammed Y.Shareef BDS, MSc., Ph.D. ⁽²⁾

Maher K. Ali BSc, MSc., Ph.D. ⁽³⁾

R.Van Noort BDS, MSc., Ph.D. ⁽⁴⁾

Key words

hydroxyapatite,
zirconia, biaxial
flexural strength,
sintering
temperature.

Abstract

The aim of this study is to investigate the effect of addition of ZrO₂ on the biaxial flexural strength (BFS) of ceramics fabricated using a conventional powder technology. Various compositions of hydroxyapatite (HAp) Ca₁₀(PO₄)₆(OH)₂ and zirconia powder ZrO₂, ranging from 10 to 90 wt% ZrO₂, were prepared using a wet mixing process. Ten compacts (13.5mm×3mm) were made for each group, pressed and sintered in air at sintering temperatures from 1100 to 1450°C for up to 12 hours. The bulk density, porosity, linear shrinkage and BFS. The porosity reduced and linear shrinkage increased with increasing sintering temperature and amounts of zirconia, whereas the sintering time had little effect. The highest mean value achieved for the BFS was 269±20 MPa for a composition of 70% ZrO₂ and 30% HAp fired at 1450°C for 6 hours. From the experimental results can be conclude that sintering temperature and composition affect densification behaviour of calcium phosphate/ ZrO₂ composites. The BFS increases with a reduction of porosity and increases with both sintering temperature and additions of ZrO₂. It was noted that there is considerable scope for improvement in the BFS values by reducing the porosity of these composites.

Introduction

Hydroxyapatite (HAp) with the chemical composition Ca₁₀(PO₄)₆(OH)₂ has been extensively study as a bone substitute. It shows an excellent biocompatibility when implanted in either soft tissue ⁽¹⁻³⁾, or hard tissue ^(4,5-7) and can form strong and intimate bond with bone ^(3,5,6). Driskell *et al.* ⁽⁸⁾ was the first to report that a chemical bond exists between bone and HAp. HAp, when sintered at high temperatures up to 1250 °C, was initially

believed to be non-resorbable ⁽¹⁾. However, it is currently generally accepted that degradation of HAp can occur to a certain extent ^(4,9). LeGeros *et al.* ⁽¹⁰⁾ reported that the bioactivity of HAp may be related to its dissolution rate. HAp is mechanically weak and unsuitable for use in stress bearing areas. Two approaches have been explored to overcome this problem ^(11,12). One of the most promising applications of calcium phosphate technology revolves around the use of HAp coatings on conventional metallic prostheses. Among the advantages of this approach is the potential for stronger, more permanent fixation of the metal implant directly to surrounding bone via HAp bone-bonding

(1)Ass. Prof., Department of Restorative Dentistry, School of Clinical Dentistry, University of Sheffield, UK.

(2)Ass. Prof., Department of Restorative Dentistry, School of Clinical Dentistry, University of Sheffield, UK.

(3)Ass. Professor, Department of Chemistry, College Faculty of Science, University of Zakho.

(4)Ass. Prof., Department of Restorative Dentistry, School of Clinical Dentistry, University of Sheffield, UK.

and the elimination of leaching of metallic trace elements into adjacent tissues. In the case of major orthopaedic appliances such as total hips and knees, a strongly adherent HAp coating on the metallic devices could obviate the need for methyl methacrylate bone cement, which has proved to be the limiting factor in long-term survival of such devices. However, all commonly used coating techniques depend on mechanical adhesion (rather than a chemical bond) to the underlying metal which makes this metal-HAp interface the weakest point of the system^(13,14). Ducheyne *et al.*⁽¹¹⁾ used HAp as surface layer on titanium implants, but this approach has several problems that include separation of the coating layer from the underlying bioinert matrix and the coating process can reduce the strength of the bioinert materials⁽¹²⁾. In vivo studies^(15,16) have assessed bony adaptation to HAp-coated and non-coated pure titanium control implants. One study demonstrated an increased amount of direct bone to implant contact with coated specimen at six weeks⁽¹⁶⁾. Sharp edges or deep threads observed on the base metal also reduce the adherence properties of these ceramics. Another concern is the dissolution of improperly applied coatings with time, and consequences that both bond strength and coating integrity will be affected^(13,15-17). The second approach is to produce HAp/Ceramic composite with better mechanical properties with HAp^(11,18) such as ZrO₂-HAp, Ti-HAp, Al₂O₃-HAp composites. The even distribution of the apatite phase as islets in a strong matrix may contribute to mineralization and direct bone apposition onto this type of ceramic composite^(18,19,12). In a study performed by Jianguo *et al.*⁽²⁰⁾, a range of high-strength hydroxyapatite composites (HAp/Oxide of Alumina, Titania or Zirconia) as well as pure hydroxyapatite, alumina, titania and zirconia were densified by hot isostatic pressing. The mechanical evaluation showed that the strength of the composite materials was 3-8 times higher than that of pure hydroxyapatite and close to that of the corresponding pure oxide. Histological evaluation under the light microscope showed direct contact between bone and ceramics for all ceramic materials studied

except for alumina. The measured bond strengths in this experiment increased in the following order: alumina, titania, zirconia/hydroxyapatite, alumina/hydroxyapatite, titania/hydroxyapatite, hydroxyapatite. Kasuga *et al.*⁽²¹⁾ reported on a glass-ceramic (apatite/wollastonite) toughened with zirconia which were prepared for widespread prosthetic applications. The strength of the composite increased with increasing zirconia content. This bioceramic exhibited extremely high bending strength (400-1000 MPa) for 30-80 vol.% ZrO₂. The bioactivity of these zirconia toughened glass-ceramic composites was evaluated by their bond strength to living bones, and it was found that the bond strength of composite containing 30 vol.% zirconia was as high as that of the glass-ceramic. Recently investigators have demonstrated that the mechanical reliability of HAp can be improved by reinforcing HAp with Al₂O₃⁽²²⁻²⁷⁾. The main problems in producing dense composites in this system are connected with the big difference in sintering temperature of the components, the enhanced tendency of HAp to decompose during sintering and the consequent interaction between HAp and reinforced phase. An attempt at producing an HAp/Al₂O₃ composite⁽²⁸⁾ sintered at 1400°C in air, resulted in the formation of calcium aluminates, due to decomposition of hydroxyapatite into tri Calcium phosphate TCP and CaO with H₂O vapour. CaO then reacted with alumina to form calcium aluminates. Several researcher have reported^(29,30-32) on hydroxyapatite-zirconia composites with different volume ratio of zirconia particles. Most of these works reflect the difficulties of retaining the HAp and ZrO₂ phases in the composites due to difference in densification temperature (e.g. HAp start to densify at 1250°C, whereas ZrO₂ start to densify at 1400°C), and decomposition of HAp at 1400°C into TCP. As a consequence the desirable initial phases cannot be preserved in the composites unless expensive high technology processing at temperatures as low as 1250°C is used. Suda *et al.*⁽²⁹⁾ produced composite ceramic contained either 1.6 or 50% of ZrO₂ by volume addition to HAp,

using cold isostatic pressure (CIP), then fired at 1300-1450°C in air atmosphere for one hour. Although the bending strength of their composite is 220-270 MPa, and the fracture toughness is 3.6-4.5 MPa.m^{1/2}. The fact that they sintered their materials at sintering temperatures higher than 1250°C, it has to be concluded that the materials obtained could not possibly be HAp/ZrO₂ composites. Takagi *et al.*⁽¹²⁾ produced HAp/ZrO₂ composites using hot isostatic pressing (HIP) at 800-1150°C at 100 MPa for 2 hours. No phase change was found in zirconia nor in the HAp phase. The strength and the toughness achieved were respectively 190 MPa and 2.3 MPa.m^{1/2}. These value were approximately 20% and 100% higher than the corresponding value for hydroxyapatite ceramics without zirconia. Li *et al.*⁽³³⁾ also used(HIP) at (1225°C at 160 MPa for 1 hour) to produce HAp/ZrO₂ composite that has excellent fatigue resistance in addition to high strength, but they did not characterised the fired composite.

The Aim of Present Work

The objective of this study concerned with structural ceramics is the generation of materials having high reliability. To achieve this objective, there are two fundamentally different approaches: flaw control and toughening. The flaw control approach accepts the brittleness of the material and attempts to control the large extremes of processing flaws. The toughening approach attempts to create microstructures that impart sufficient fracture resistance so that the strength becomes insensitive to the size of flaws. The former has been the subject of considerable research that identifies the most detrimental processing flaws, as well as the processing step responsible for those flaws⁽³⁴⁻³⁶⁾. The latter has emerged more recently, and has the obvious advantage that appreciable processing and post processing damage can be tolerated without compromising the structural reliability⁽³⁶⁻³⁸⁾. The objective of this study is to develop a bioactive, high strength and toughened calcium phosphate/ZrO₂ composite, which can be used in load bearing applications.

Materials and Methods

Hydroxyapatite (HAp) and ZrO₂ powders were used in this study, supplied by Plasma Biotol Ltd, Tidswell, and Unitec Ceramics, Stafford, UK respectively. The particles size of both powders were determined using a laser diffraction method. The bulk density, true porosity, linear shrinkage and BFS were determined for the sintered samples. The bulk density values were calculated using the following equation:

$$\text{Bulk Density} = \frac{\text{Weight (g)}}{\text{Bulk Volume (cm}^3\text{)}} \dots\dots\dots(1)$$

Hence, $\text{Bulk Volume} = r^2h\pi$, where r and h are the compact's radius and height respectively.

The % theoretical density values were calculated using the bulk density of the compacts and the theoretical density value for HAp and zirconia of 3.156 and 6.05 g.cm⁻³ respectively^(39,40,41), as follow:

$$\text{Theoretical Density (\%)} = \frac{\text{Bulk Density (g.cm}^{-3}\text{)}}{\text{Theoretical Density (g.cm}^{-3}\text{)}} \times 100 \dots\dots(2)$$

Also, the true porosity values were calculated using the following formula:

$$\text{Total Porosity (\%)} = 1 - \frac{\text{Bulk Density (g.cm}^{-3}\text{)}}{\text{Theoretical Density (g.cm}^{-3}\text{)}} \times 100 \dots\dots\dots(3)$$

The linear shrinkage values of the fired compacts were determined by measuring the initial and the fired diameters of each sample as follow:

$$\text{Linear Shrinkage (\%)} = \frac{D_i - D_f}{D_i} \times 100 \dots\dots\dots(4)$$

Where, D_i and D_f are the initial and the fired diameter of the compact.

The BFS for a range of firing schedules of each HAp and ZrO₂ powder was determined for 10 test-samples. The surface of the test-samples were made flat by grinding with 600 grit SiC paper to avoid an uneven load. Each test-samples was placed on an annular knife edge of

9 mm diameter and then loaded in an universal testing machine with a cross-head speed of 0.5mm/min (Lloyd M5K). The compacts were loaded to fracture and the maximum load was recorded. The BFS was calculated using the following formula⁽⁴²⁾:

$$\sigma_f = \frac{P}{h^2} \{0.606 \ln(a/h) + 1.13\}$$

..... (5)

where σ_f is the BFS, P is the load to fracture, a is the radius of the knife-edge support and h is the sample thickness. Fracture toughness values of hot pressed HAp, 30:70 vol.% HAp: ZrO₂-U composite and ZrO₂-U samples were evaluated.

Results

4.1 Characteristics Properties of the Starting Powders

The particles size analysis using laser diffraction method showed that the mean particle size of ZrO₂ sample coded-U was 0.5 μ m and ZrO₂ sample coded-M was 1.6 μ m. The main characteristics properties of the starting powders of HAp have been reported earlier⁽⁴³⁾.

4.2 Sintering Behaviour of the Fired Samples

The sintering behaviour of the fired HAp samples for the theoretical density, linear sintering shrinkage and the BFS have been reported previously by Shareef *et al.*⁽⁴³⁾, whereas for the fired samples prepared from ZrO₂ sample coded-U and ZrO₂ sample coded-M used in this study are presented in Figs. 1, 2, and 3. These were found increasing of theoretical density, Linear Shrinkage and BFS with increasing the sintering temperature. The sintering behaviour of the fired HAp/ ZrO₂ composite for the theoretical density, linear firing shrinkage and the BFS values were plotted against sintering temperature, time and addition of ZrO₂ as shown in Figs. 4, 5 and 6. These were found increase with increasing sintering temperature, time and addition of ZrO₂. As shown in Fig. 6, the highest mean value achieved for the BFS was 269 \pm 20 MPa for a composition of

70% ZrO₂-U, fired at 1450°C for 6 hours, because the densification process reached to the highest fired density and resulting lower porosity value as shown in Table 1. However, with the hydroxyapatite (HAp) decomposed to α -TCP. On the other hand the fracture toughness values for the hot pressed samples prepared from HAp, HAp/ ZrO₂ composite and ZrO₂ are plotted against the materials used as shown in Fig. 7. Also, the main values of the BFS, fracture toughness and the fired theoretical density are shown in Table 2.

Discussion

It has been found that, by increasing the sintering temperature, time and addition of ZrO₂, the theoretical density and linear shrinkage values were increased for the HAp/ ZrO₂ composites. This cause an increase in the BFS values because the densification process increased with increasing these factors (Figs. 1, 2 and 3). The same observation has been found by Takagi *et al.*⁽¹²⁾, which is stated that the densification behaviour of HAp/ ZrO₂ composite increased with increasing firing temperature and the amount of zirconia content. The development of HAp toughened materials by dispersed zirconia particles has been found difficult as reported by Evans^(35,36) and Wu *et al.*⁽¹⁸⁾. One major obstacle has been found the reaction between the matrix and dispersed particles during the sintering process. Calcium which is the major constituent of HAp, diffuse into ZrO₂ and change it to stable cubic phase, for which a transformation toughening mechanism is not expected to occur as reported by Takagi *et al.*⁽¹²⁾. To avoid the difficulty associated with the diffusion, the temperature for densification has to be minimised. However, this is difficult because the composites generally have inferior sintering characteristics, and require high temperature for densification. Takagi *et al.*⁽¹²⁾ achieved considerable reduction of densification temperature in a composite ceramics containing ZrO₂ particles dispersed in HAp using combined application of a colloidal pressing technique and densification by hot isostatic

pressing. The biocompatibility of the reinforcement phase should also be considered when the ceramic matrix composite is designed to be involved in biomaterials applications. Most metals react with the HAp to form metal oxides and tri-calcium phosphate [TCP, Ca₃(PO₄)₂] or tetra-calcium phosphate (TeCP, Ca₄(PO₄)₂O), leading to a serious reduction in the biocompatibility of HAp. Partially stabilized zirconia has been commonly used as reinforcement for many ceramics because of its high strength and fracture toughness. Bioinertness is another merit of the ZrO₂. However, extensive reaction between the HAp and the ZrO₂ to form TCP and fully stabilized ZrO₂ is a big disadvantage of this approach. The calcium phosphate/ ZrO₂ composite obtained in this study was contained approximately 5% porosity. Further work is needed by using a hot pressing technique and reducing the

particles size to enhance the uniformity of the micro structures of the composite. This will eliminate the porosity on one hand and to reduce the sintering temperature on the other hand to level which keeps HAp thermally stable at certain sintering temperatures as reported earlier by Shareef *et al.* ⁽⁴³⁾.

Conclusions

1. Sintering temperature and addition of ZrO₂ were affected the densification behaviour of HAp/ ZrO₂ composite, whereas the firing time had little effect.
2. The BFS values were increased with an increase both sintering temperature and additions of zirconia.
3. There is considerable scope for improvement in the BFS and fracture toughness values by reducing the porosity and the particles size of these composites.

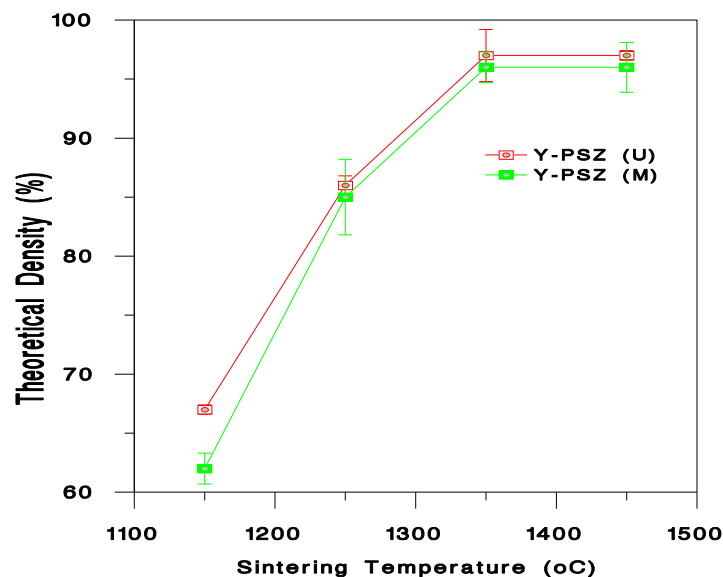


Fig. (1):- The effect of sintering temperature on the % theoretical density of ZrO₂-U and ZrO₂-M samples, fired for 6 hrs in an air atmosphere (Y-PSZ is yttrium partially stabilised zirconia).

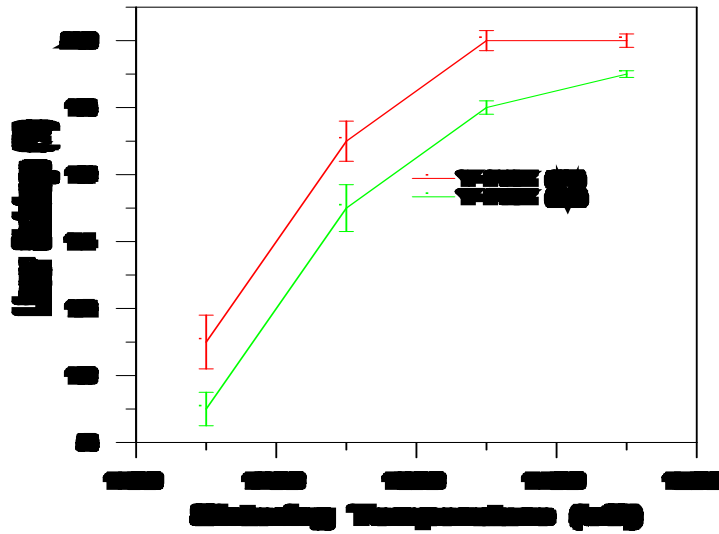


Fig. (2):- The effect of sintering temperature on the % linear shrinkage of ZrO₂-U and ZrO₂-M samples, fired for 6 hrs in an air atmosphere (Y-PSZ is yttrium partially stabilised zirconia).

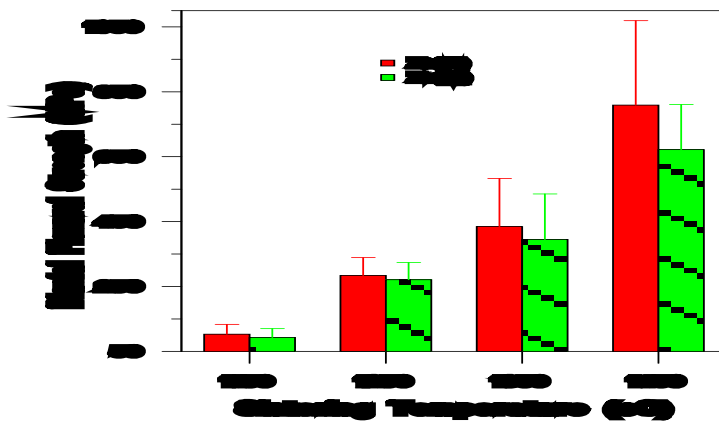


Fig.(3):- The effect of sintering temperature on the BFS of ZrO₂-U and ZrO₂-M samples, fired for 6 hrs in an air atmosphere.

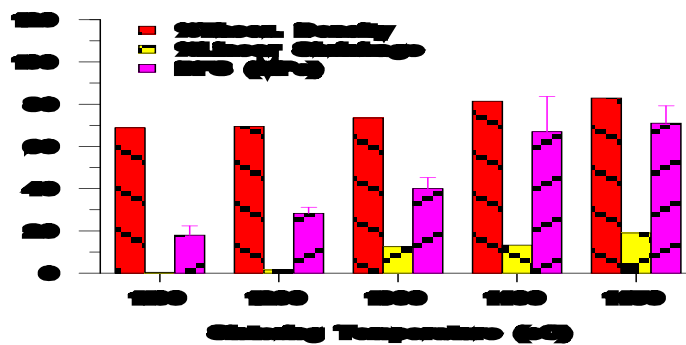


Fig.(4):- Theoretical density, Linear shrinkage and BFS plotted as a function of sintering temperature for samples prepared from composite of 45:55 vol.% HAp:ZrO₂-U fired for 6 hrs.

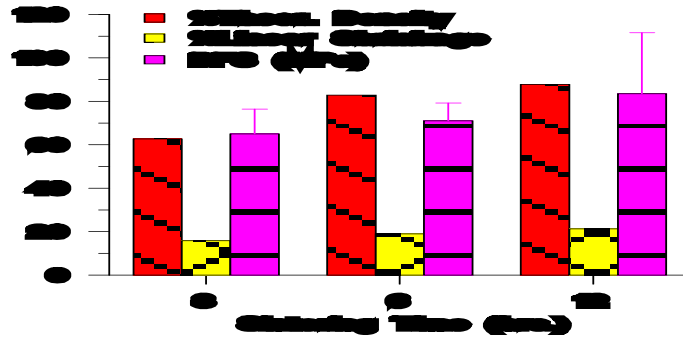


Fig.(5):- Theoretical density, linear shrinkage and BFS plotted as a function of sintering time for samples prepared from composite of 45:55 vol.% HAp:ZrO₂U composite fired at 1450°C.

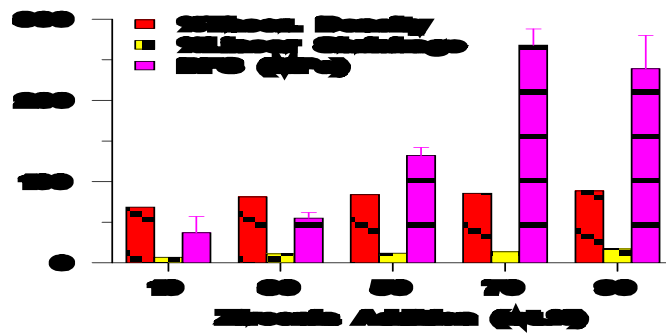


Fig.(6):- Theoretical density, linear shrinkage and BFS plotted as a function of zirconia addition, fired at 1450°C for 6 hrs.

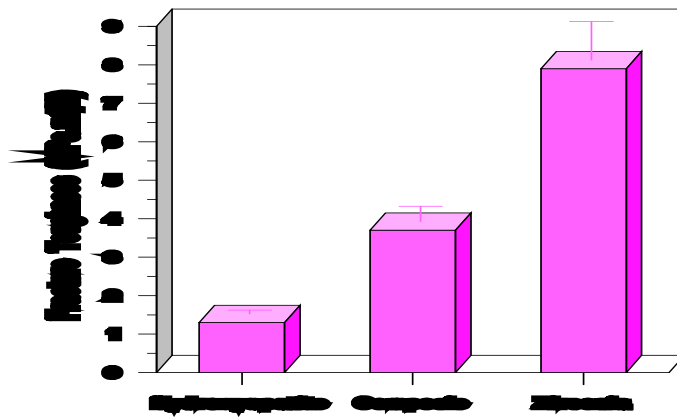


Fig. (7):- Fracture toughness of hot pressed HAp, 30:70 vol.% HAp:ZrO₂-U composite and ZrO₂-U samples

Table (1):- BFS and % theoretical density data of composite prepared from composition of 30:70 vol.% HAp:ZrO₂-U.

Parameters	HAp/ ZrO ₂ -U	HAp/ ZrO ₂ -M
BFS (MPa)	20±269	10±176
% Theoretical Density	0.5±95	0.8±85
% True Porosity	5	15

Table (2):- The main values of BFS, fractures toughness and the fired theoretical density of hot pressed HAp, HAp:ZrO₂-U composite and ZrO₂-U ceramics.

Parameter	HAp	30:70 vol.% (HAp: ZrO ₂)	ZrO ₂
BFS (MPa)	17±142	19±269	223±1213
Fracture Toughness (MPa.m ^{1/2})	0.1±1.3	0.4±3.8	1.0±8.2
%Theoretical Density	4±94	0.5±95	0.8±99

References

- 1-Ogiso, M., Kaneda, H. Arasaki, J and Tabata, T., "Epithelial attachment and bone tissue formation on the surface of hydroxyapatite ceramics dental implants", In: Biomaterials 1980, Winter GD et al. (eds), John Wiley and Sons Ltd, London, 1982:59-64.
- 2-Jansen, J.A., de Wijn J.R., Wolters-Lutgerhorst, JML and van Mullem PJ, "Ultrastructural study of epithelial cells attachment to implant materials", J. Dent. Res. 1985; 64: 891-896.
- 3-Van Blitterswijk, C.A., Hesselings, S.C., Grote, J.J., Koerten, H.K. and de Groot, K., "The biocompatibility of hydroxyapatite ceramic: A study of retrieved human middle ear implants", J. Biomed. Mater. Res. 1990; 24: 433-453.
- 4-Van Blitterswijk, Grote J.J., Kwijpers C.J.G., van Hock B. and Daems W.T.H. "Bioreactions at the tissue hydroxyapatite interface", Biomaterials, 1985; 6: 241-251.
- 5-Jarcho, M. Kay, J.F. Kenneth, I. Gumaer, K.I. Doremus, R.H. and Drobeck, H.P., "Tissue cellular and subcellular events at a bone-ceramic hydroxyapatite interface", J. Bioeng. 1977; 1: 79-92.
- 6-Denissen, H. W., de Groot, K., Makkes, PCh, van den Hoff, A. and Klopper, P.J., "Tissue response to dense apatite implants in rats", J. Biomed. Mater. Res. 1980; 14: 713-721.
- 7-De Groot, K. Degradable ceramics, In:" Biocompatibility of implant materials", Williams, D.F. (ed), CRC Press, Boca Raton, FL, USA, 1981; 1: 199.
- 8-Driskell, T.D., Hassler, C.R., Tennery, V.J., McCoy, I.R. and Clarke, W.J., "Calcium phosphate resorbable ceramic: a potential alternative for bone grafting", J. Dent. Res. 1973; 52: 123-131.
- 9-Van Blitterswijk, C.A. and Grote, J.J., "Biological performance of ceramics during inflammation and infection", In: CRC Critical Reviews in Biocompatibility, 1989; 5: 13-43.
- 10-LeGeros, R. Z., Daculsi, G. Orly, I. Gregoire, M. Heughebaert, M. Gineste, M. and Kijkowska," Formation of carbonate apatite on calcium phosphate materials: Dissolution/precipitation processes", In: Bone-bonding biomaterials, Ducheyne P. et al. (Eds), Reed Healthcare Communications, Leiderdorp, The Netherlands, 1992; 201-112.
- 11-Ducheyne, P., Hench, L.L., Kagan, A., Martens, M., Burssens, A., and Mulier, J.C.;" Effect of hydroxyapatite impregnation on skeletal bonding of porous coated implants", J. Biomed. Mater. Res. 1980; 14: 225-337.
- 12-Takagi, M., Mochida, M., Uchida, N., Saito, K. and Uematsu, K.," Filter cake forming and hot isostatic pressing for TZP-dispersed hydroxyapatite composite", J. Mater. Sci.: Mater. Med. 1992; 3: 199-203.
- 13-Ellies, L. G., Nelson, D.G.A., Featherstone, J.D.B., "Crystallographic changes in calcium phosphate during plasma spraying", Biomaterials 1992;13: 313-316.
- 14- Jarcho, M.," Retrospective analysis of hydroxyapatite development for oral implant applications", Dent. Clin. N. Am. 1992; 36: 19-26.
- 15-Hayashi, K., Matsuguchi, N., Uenoyama, K., Kanemaru, T. and Sugioka, Y., "Evaluation of metal implants coated with several types of ceramics as

- biomaterials", *J. Biomed. Mater. Res.*, 1989; 23: 1247-1259.
- 16-Gottlander, M., Albrektsson, T., "Histomorphometric studies of hydroxyapatite-coated and uncoated CP titanium threaded implants in bone", *J. Oral Maxillofac. Implants*. 1991; 6: 399-404.
- 17-Kay, J. F., "Calcium phosphate coatings for dental implants. Current status and future potential", *Den. Cl. N. Am.*, 1992; 36: 1-18.
- 18-Wu, J-M. and Jeh, T-S., "Sintering of hydroxyapatite-zirconia composite materials", *J. Mater. Sci: Mater. Med.* 1988; 23: 3771- 3777 .
- 19-Li, J., Hermansson, L. and Soremark, R., "High-strength biofunctional zirconia: mechanical properties and static fatigue behaviour of zirconia-apatite composites", *J Mater. Sci: Mater. Med.* 1993; 4: 50-54.
- 20-Jianguo, Li. and Bahman, Fartash," High-strength bioactive ceramic composite In: *Biomaterial-Tissue Interface*", Doherty., P.J. et al. (eds)., *Advance in Biomaterials*, Elsevier Science Publishers B.V. 1992;10.
- 21-Kasuga, T., Yoshida, M., Ikushima, A. J., Tuchiya, M. and Kusakari, H., "Stability of zirconia-toughened bioactive glass-ceramics: in vivo study using dogs", *J. Mater. Sci.: Mater. in Med.* 1993; 4: 36-39.
- 22-Hayashi, K., Matsuguchi, N., Uenoyama, K. and Sugioka, Y. "Re-evaluation of the biocompatibility of bioinert ceramics in vivo", *Biomaterials*, 1992; 13 (4):195-200.
- 23-Huaxia, Ji., and Marquis, P.M., "Preparation and characterization of Al₂O₃ reinforced hydroxyapatite, *Biomaterials*, 1992; 13(11): 744-748.
- 24-Dimitrova-Lukacs, M. and Gillemot, L., "Bioactive-Bioinert Composite Bioceramics", in 3rd *Euro-Ceramics* Duran, P. and Fernandez, (eds), Iberica S.L. Faenza Spain, 1993; 3.
- 25-Dimitrova-Lukacs, M., "Sintered bioactive-bioinert ceramic composites", *Biomaterial meeting*, Sheffield, 1994.
- 26-Dimitrova-Lukacs, M., "Mechanical Properties of hydroxyapatite/fluorapatite-alumina composites", *Biomaterial meeting*, Sheffield, 1994.
- 27-Rieu, J. and Goeuriot, P., "Ceramic composites for biomedical applications", *Clinical Materials*, 1993; 12: 211-217.
- 28-Terry B.C., Albright J.E. and Baker R.D., "Alveolar ridge augmentation in the edentulous maxilla with use of autologous ribs", *J. Oral Surg.* 1974; 32: 429-433.
- 29-Suda, A., Sato, T., Takagi, M. and Osanai, T., "Biocompatibility of zirconia dispersed hydroxyapatite ceramics", *J. Jpn. Orthopaedic Assoc.*, 1990; 64: 249-259.
- 30-Garvie, R.C. and Nicholson, P.S., "Phase analysis in zirconia systems", *J. Am. Ceram. Soc.*, 1972; 55: 303-305.
- 31-Garvie, R. C., Hannink, R. H. and Pascoe, R. T., "Ceramic steel. *Nature*", (London), 1975;258: 703-704.
- 32-Lange F.F., Shubert, H., Claussen, N. and Ruhle, M., "Effects of attrition milling and post sintering heat treatments on fabrication, microstructure and properties of transformation toughening ZrO₂", *J. Mater. Sci.* 1986; 21: 768-774.
- 33-Denissen, H.W., Veldhuis, A.A. H., Makkes, P.C., et al., "Dense apatite implants in preventive prosthetic dentistry", *Clin. Prevent. Dent.*, 1980; 2: 23-28.
- 34-Large, F. F., "Powder processing science and technology for increased reliability", *J. Am Ceram. Soc.*, 1989; 72(1): 3-15.
- 35-Evans, A. G., "Structural reliability: Processing dependent phenomenon", *J. Am. Ceram. Soc.* 1982; 65(3): 127-137.
- 36-Evans, A. G., "New opportunities in the processing of high reliability structural ceramics pp 989-1010 in *ceramic transactions*, vol. 1, ceramic powder science Edited by Messing, G. and Hausner, H. *Am. Ceram. Soc.*, Westerville, OH, 1989.
- 37-Cook, R. F., Lawn, B. R. and Fairbanks, C. J., "Microstructure strength properties in ceramics: I, Effect of crack size on toughness", *J. Am. Ceram. Soc.*, 1985; 68(11): 604-615.
- 38-Marshall, D. B. Strength characteristics of transformation toughening zirconia, *J. Am. Ceram. Soc.* 1986; 69(3): 173-180.
- 39-Shareef, M. Y., Messer, P. F. and van Noort, R., "Fabrication of Machineable Hydroxyapatite", *Br. Ceram. Proc.* 1990; 45: 59-70.
- 40-Shareef, M., "Fabrication, characterisation and fracture behaviour of machinable hydroxyapatite ceramics", Ph.D thesis, Sheffield University, 1991.
- 41-Richerson, D. W., "Modern ceramic engineering: Properties, processing and use in design", 2nd Ed., Marcel Dekker, New York., 1992.
- 42-Shareef, M.Y., van Noort, R. Messer, P.F. and Piddock, V., "The effect of microstructural features on the biaxial flexural strength of leucite reinforced glass-ceramics", *J. Mater. Sci.: Mat. Med.* 1994; 5(2): 113-118.
- 43-Shareef, M.Y., Hassen, M.A. and Maher, K.A., "Effect of heat treatment and phase change on BFS of two hydroxyapatite ceramic powders", *Iraqi National Journal of Chemistry*, 2011;44:526-538.